
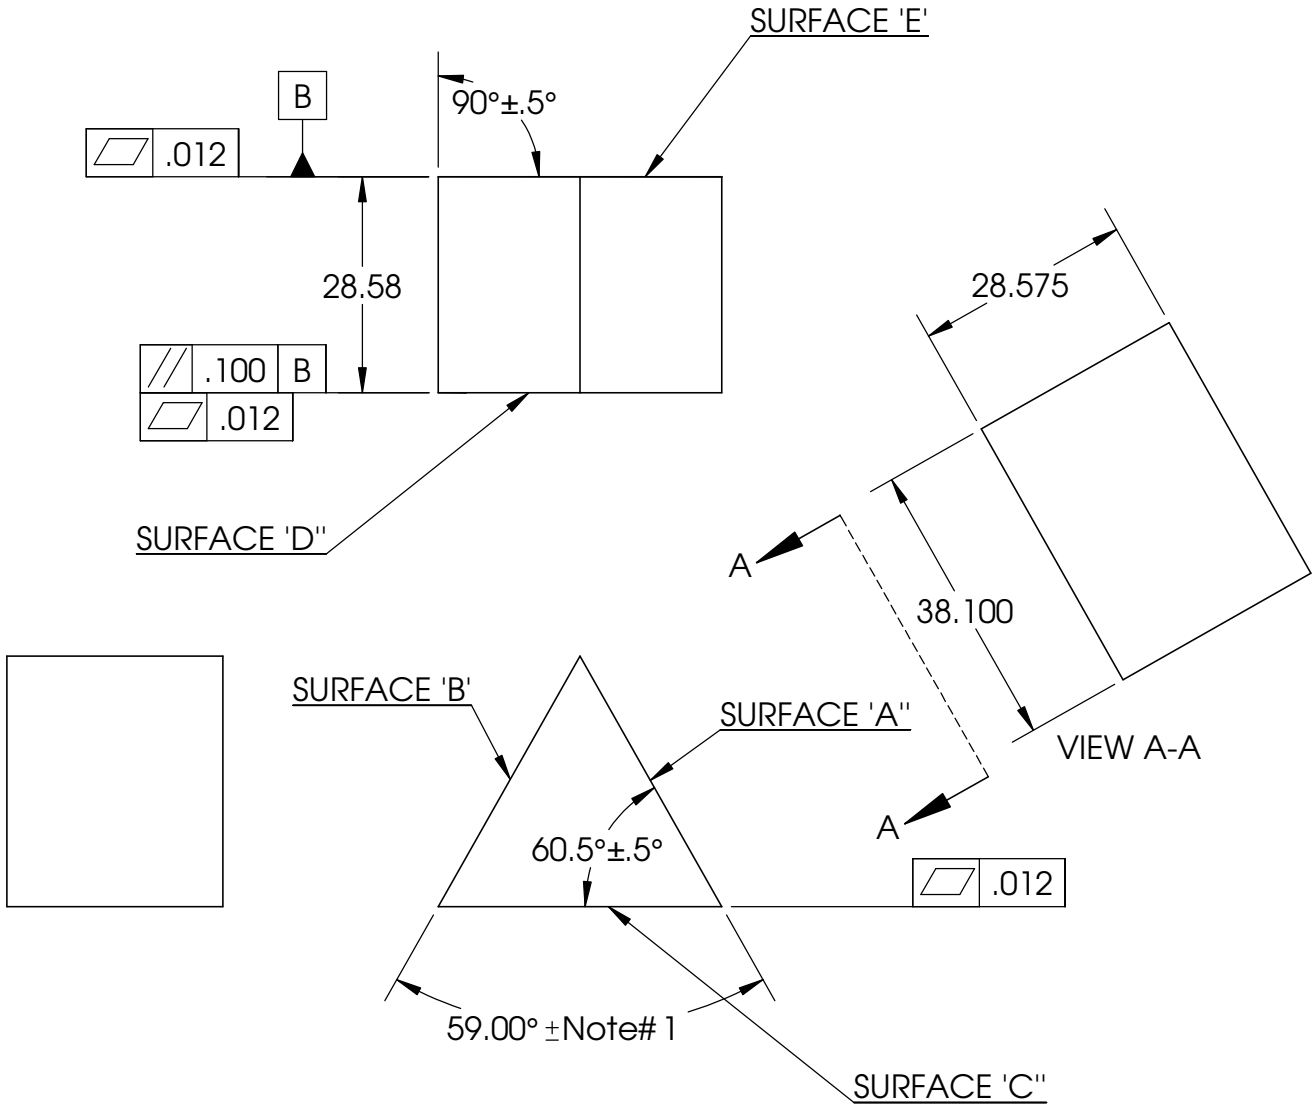


SIDES 'A' and 'B' SHALL MEET THE BELOW SPECIFICATIONS	
Irregularity:	1/4 FRINGE
Power:	1/4 FRINGE
Clear Aperture:	80%
Surface Quality:	80-50
Bevels:	.20mm to 1 mm
Fringes measured @ 633nm	

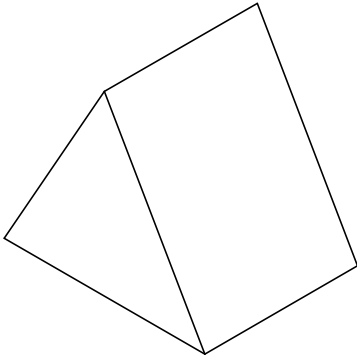

NOTES:

1. EQUATION:
2. PYRAMID ERROR OF SURFACE 'D' WITH RESPECT TO SURFACES 'A' AND 'B' 5 ARC MINUTES MAX
3. PYRAMID ERROR OF SURFACE 'E' WITH RESPECT TO SURFACES 'A' AND 'B' 5 ARC MINUTES MAX

PROPRIETARY

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF **M³ Measurement Solutions Inc.**, ANY REPRODUCTION IN PART OR IN WHOLE WITHOUT THE WRITTEN PERMISSION OF **M³ Measurement Solutions Inc.**, IS PROHIBITED

	NAME	DATE
DRAWN		
CHECKED		
ENG APPR.		
MFG APPR.		
DIMENSIONS ARE IN INCHES TOLERANCES: ANGULAR: ± 0.5 TWO PLACE DECIMAL $\pm .15$ THREE PLACE DECIMAL $\pm .02$		



M³ Measurement Solutions Inc
2048 Aldgrove Suite D
Escondido, CA 92029
WEB: WWW.M3MSI.COM

INDEX SAMPLE

SIZE A	DWG. NO. INDEX SAMPLE	REV.
SCALE: 1:1	WEIGHT:	SHEET 1 OF 1